

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0056
Location:	LONG BRANCH POLICE DEPT		
Calibration File No.:	00545	Calib. Date:	10/16/2015
Certification File No.:	00546	Cert. Date:	10/16/2015
Linearity File No.:	00547	Lin. Date:	10/16/2015
Solution File No.:	00560	Soln. Date:	01/06/2016
Sequential File No.:	00560	File Date:	01/06/2016

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXN S3-0217
Control Solution %:	0.100%			Expires:	08/04/2017
Solution Control Lot:	15H140			Bottle No.:	1341

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:06S		
Control 1 EC	0.099%	21:07S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	21:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:08S		
Control 2 EC	0.099%	21:08S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	21:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:09S		
Control 3 EC	0.099%	21:10S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	21:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: VALDES

First Name: HEATHER

MI: -

Signature: \_\_\_\_\_

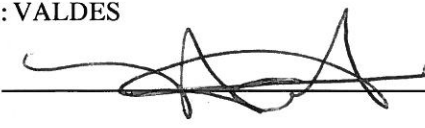

Badge No.: 290

Date: 01/06/2016