

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0056
Location:	LONG BRANCH POLICE DEPT		
Calibration File No.:	00545	Calib. Date:	10/16/2015
Certification File No.:	00546	Cert. Date:	10/16/2015
Linearity File No.:	00547	Lin. Date:	10/16/2015
Solution File No.:	00567	Soln. Date:	02/06/2016
Sequential File No.:	00567	File Date:	02/06/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXN S3-0217
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	1340

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:38S		
Control 1 EC	-.---%	06:39S	23.4°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	06:39S	23.4°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: EVANGELHO

First Name: JOHN

MI: A

Signature: _____

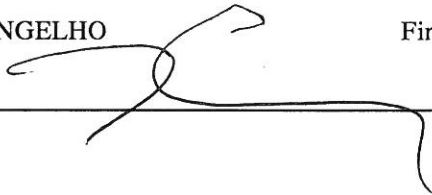

Badge No.: 274

Date: 02/06/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0056
Location:	LONG BRANCH POLICE DEPT		
Calibration File No.:	00545	Calib. Date:	10/16/2015
Certification File No.:	00546	Cert. No.:	00022
Linearity File No.:	00547	Cert. Date:	10/16/2015
Solution File No.:	00568	Lin. No.:	00017
Sequential File No.:	00568	Lin. Date:	10/16/2015
		Soln. Date:	02/06/2016
		Soln. No.:	00115
		File Date:	02/06/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXN S3-0217
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	1330

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:07S		
Control 1 EC	-.---%	08:07S	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	08:07S	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: EVANGELHO

First Name: JOHN

MI: A

Signature: _____



Badge No.: 274

Date: 02/06/2016