

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00350 Calib. Date: 11/30/2012 Calib. No.: 00015
Certification File No.: 00351 Cert. Date: 11/30/2012 Cert. No.: 00010
Linearity File No.: 00352 Lin. Date: 11/30/2012 Lin. No.: 00010
Solution File No.: 00358 Soln. Date: 03/25/2013 Soln. No.: 00073
Sequential File No.: 00358 File Date: 03/25/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXN S3-0216
Control Solution %: 0.100% Expires: 04/25/2014
Solution Control Lot: 12D101 Bottle No.: 0950

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:55S		
Control 1 EC	0.099%	15:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:56S		
Control 2 EC	0.099%	15:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	15:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:58S		
Control 3 EC	0.098%	15:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:00S		

All tests within acceptable tolerance.

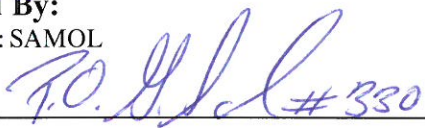
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SAMOL

First Name: GEORGE

MI: L

Signature:  #330

Badge No.: 330

Date: 03/25/2013