

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0056
Location:	LONG BRANCH POLICE DEPT		
Calibration File No.:	00629	Calib. Date:	10/21/2016
Certification File No.:	00630	Cert. Date:	10/21/2016
Linearity File No.:	00631	Lin. Date:	10/21/2016
Solution File No.:	00664	Soln. Date:	04/03/2017
Sequential File No.:	00664	File Date:	04/03/2017
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXN S3-0217
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	1326

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:38D		
Control 1 EC	0.099%	04:38D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:39D		
Control 2 EC	0.100%	04:40D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:41D		
Control 3 EC	0.099%	04:42D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:43D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

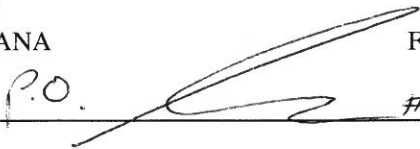
Changed By:

Last Name: UMANA

First Name: HECTOR

MI: D

Signature: _____

P.O.  # 328

Badge No.: 328

Date: 04/03/2017