

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0056
Location:	LONG BRANCH POLICE DEPT	
Calibration File No.:	00176	Calib. Date: 07/19/2010
Certification File No.:	00177	Cert. No.: 00010
Linearity File No.:	00178	Cert. Date: 07/19/2010
Solution File No.:	00219	Lin. No.: 00005
Sequential File No.:	00219	Soln. Date: 01/10/2011
		Soln. No.: 00043
		File Date: 01/10/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXN S3-0216
Solution Control Lot:	09H068	Expires: 08/05/2011
		Bottle No.: 0236

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:59S		
Control 1 EC	0.099%	05:59S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	05:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:00S		
Control 2 EC	0.098%	06:01S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:02S		
Control 3 EC	0.099%	06:02S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	06:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:03S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: GARRETT

First Name: BRIAN

MI: A

Signature: _____

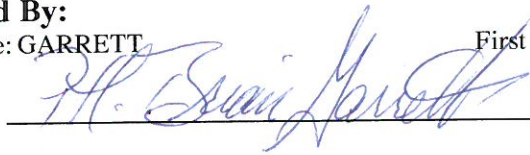

Badge No.: 306

Date: 01/10/2011