

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00256 Calib. Date: 07/05/2011 Calib. No.: 00012
Certification File No.: 00257 Cert. Date: 07/05/2011 Cert. No.: 00007
Linearity File No.: 00258 Lin. Date: 07/05/2011 Lin. No.: 00007
Solution File No.: 00268 Soln. Date: 09/02/2011 Soln. No.: 00053
Sequential File No.: 00268 File Date: 09/02/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXN S3-0216
Control Solution %: 0.100% Expires: 03/31/2013
Solution Control Lot: 11C088 Bottle No.: 1382

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:57D		
Control 1 EC	0.100%	16:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:58D		
Control 2 EC	0.100%	16:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:00D		
Control 3 EC	0.100%	17:01D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	17:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:01D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BARRETT

First Name: TRACEY

MI: L

Signature: _____

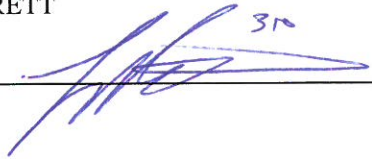

Badge No.: 310

Date: 09/02/2011